
imp De Mayo V² E[®] Knee Positioner Instructions For Use ~ STERILE Extension

1. Locate the patient's gluteal fold near the break at the end of the table.





2. Apply a well leg holder to the non-operative leg.






lower the end of the table and remove the pad.




4. To position the Clamp:

Method 1: Find the end of the rail at the break and move the Clamp proximal approximately 7 inches.

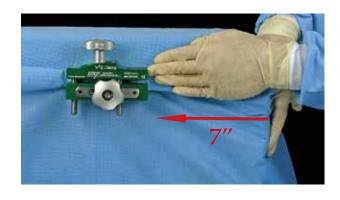



To lock the Clamp on the side rail, squeeze the jaws and tighten the top Knob.

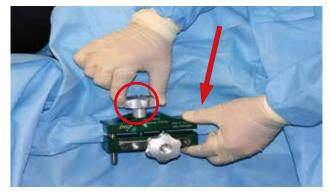



Loosen the side Knob all the way by turning it counter clockwise.



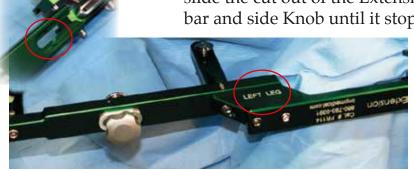







Turn the Knob clockwise to tighten.


Confirm a minimum of 2 inches of space between the end of the table and Extension.

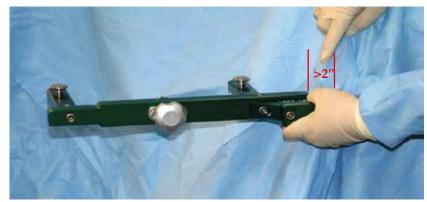

Method 2: First attach the Extension to the Clamp assuring the side Knob is completely loose by turning it counter clockwise, with the appropriate side leg showing on the Extension. Slide the cut out of the Extension over the clamp's metal bar and side Knob until it stops,

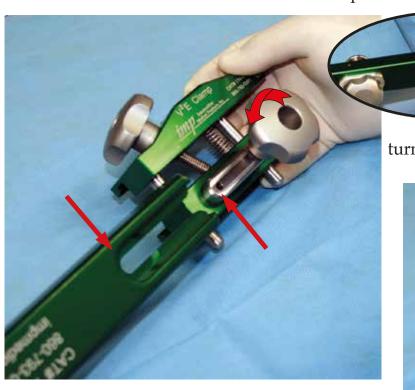


turn the Knob clockwise to tighten.

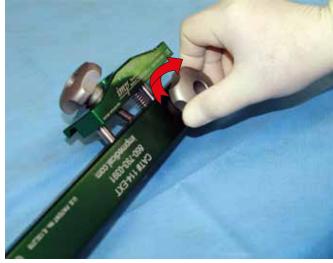

Confirm a minimum of 2 inches of space between the end of the

table and Extension.

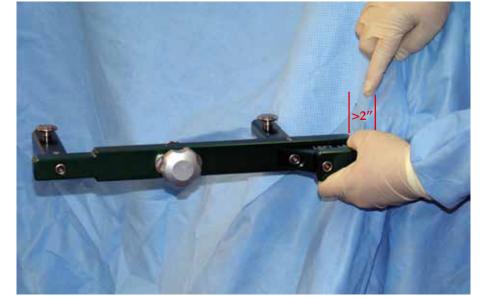

To lock the clamp to the side rail, squeeze the Jaws and tighten the top Knob.






5. Turn the spring loaded Knob counter clockwise all the way in the loose position prior to seating the Base Plate.





To seat the Base Plate on the Extention, line up the white arrows on the Base Plate and Extension.

Pull the Base Plate at an angle against the Receiver Stud and end of the spring loaded Knob.

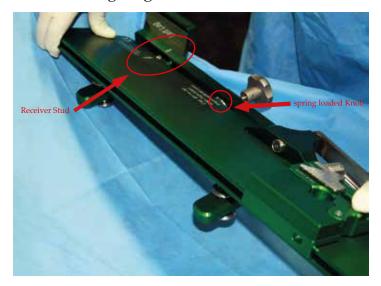

Push down on the Base Plate for final seating, and finger tighten the Knob turning clockwise.





To remove, loosen Knob all the way turning counter clockwise then pull the Base Plate and lift to remove.

6. Protect your patient from potential Pressure Ulcers. Insert the *imp* Patient Protective Pad into the sterile boot.





7. To insert the pad, position the carriage under the patient's foot with the knee flexed.






Insert the ball of the boot into the carriage and tighten the E-Brake.







For additional holding, rotate the Locking Lever to the right.

8. Place the patient's foot in the boot and wrap cohesive bandage around the foot starting with a minimum of six (6) foot wraps, tear, and finish the wrap above the bracket around the calf.







Avoid wrapping cohesive bandage over the bracket on the back of the boot.



9. To reposition the leg:Slide the varus tilt lever to Open,






unlock the E-Brake by turning it counter clockwise,





and loosen the Locking Lever by rotating to the left.






The doctor may approach the knee procedure between the legs of the patient.



Set Up Test Procedure 🔼 📜 🗓





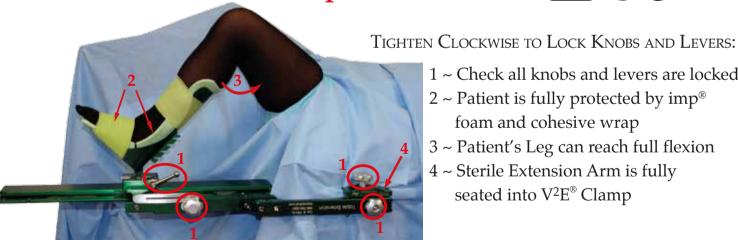

- 1 ~ Check all knobs and levers are locked
- 2 ~ Patient is fully protected by imp® foam and cohesive wrap
- 3 ~ Patient's Leg can reach full flexion
- 4 ~ Sterile Extension Arm is fully seated into V²E[®] Clamp

imp[®] Innovative

Medical Products, Inc.

87 Spring Lane, PO Box 8028

PH: (860) 793-0391 FAX: (866) 459-1805 Toll Free PH:1-800-467-4944

www.impmedical.com



imp® products are protected by patent & patent pending rights ~ go to impmedical.com/patents

Plainville, CT 06062

August 2019 Innovative Medical Products To a © August 2019 Innovative Medical Products, Inc. ALL RIGHTS RESERVED